




1000400-8040001

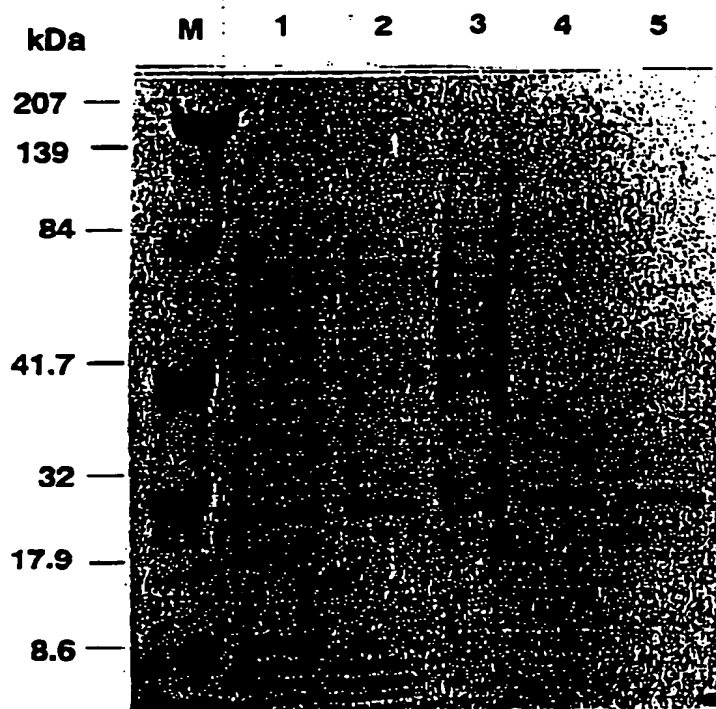

2/15

Fig.2

FOOT-804000

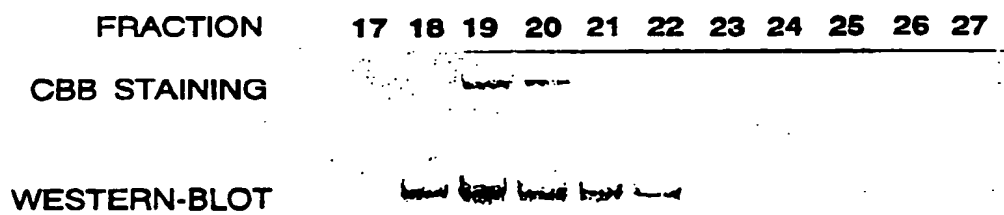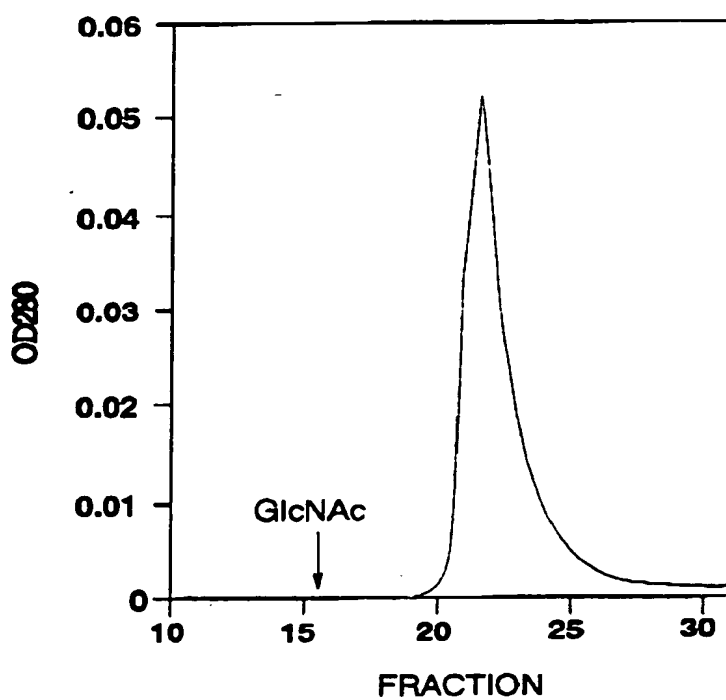


3/15

Fig.3

0.15 0.6 2.5
0 0.3 1.2 5 (mM)

203
135
81
44
32.3
17.4


103011-80420001

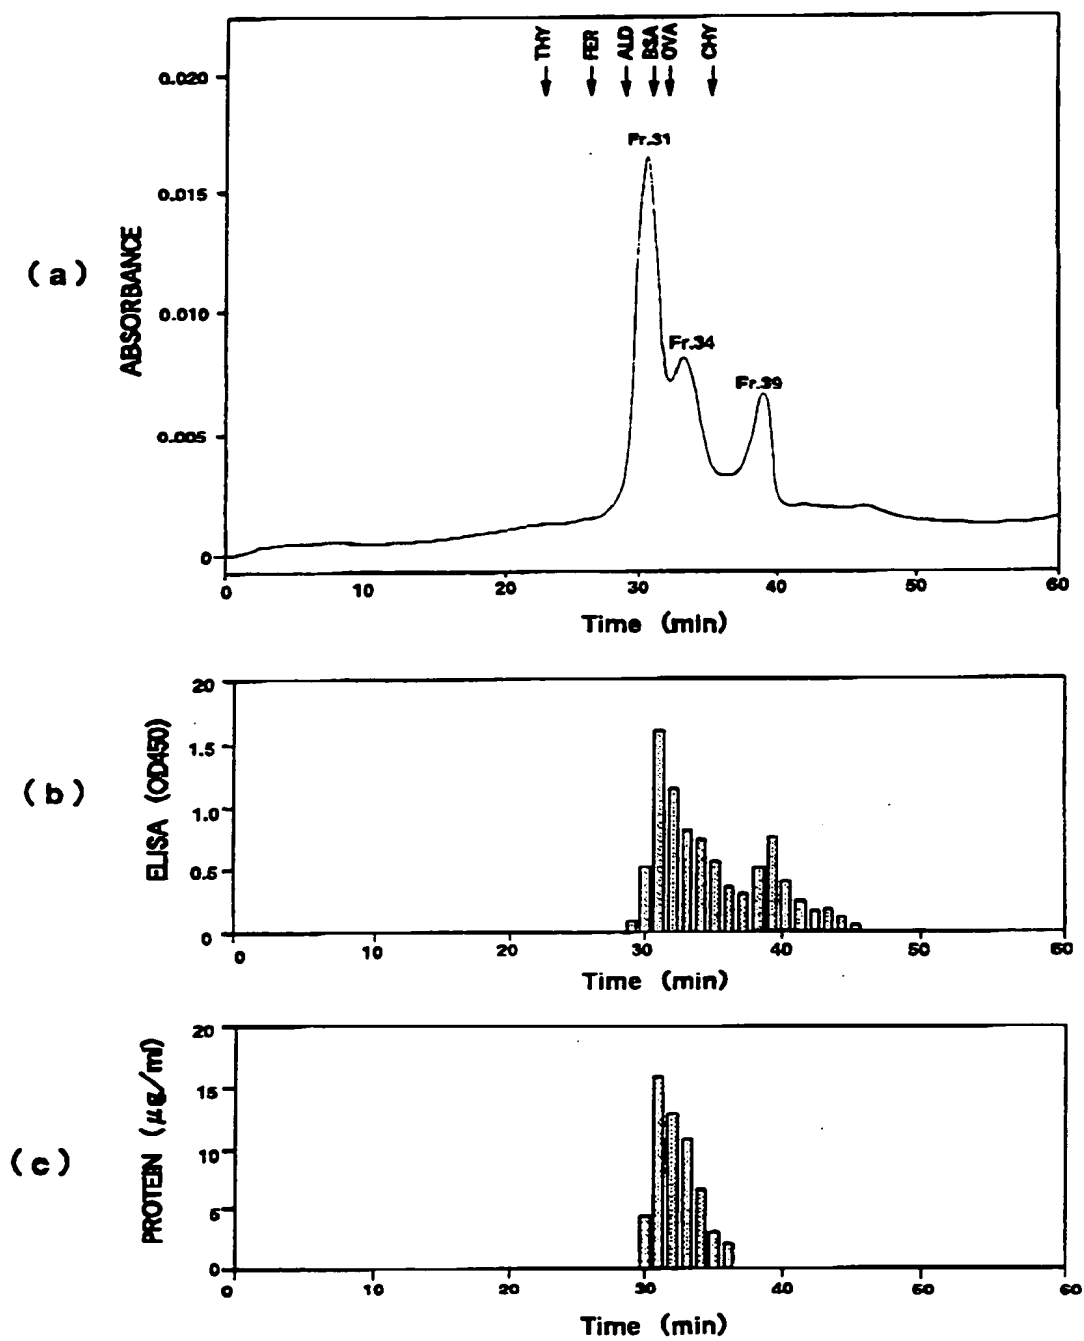


5/15

Fig.5

THE UNIVERSITY OF CHICAGO

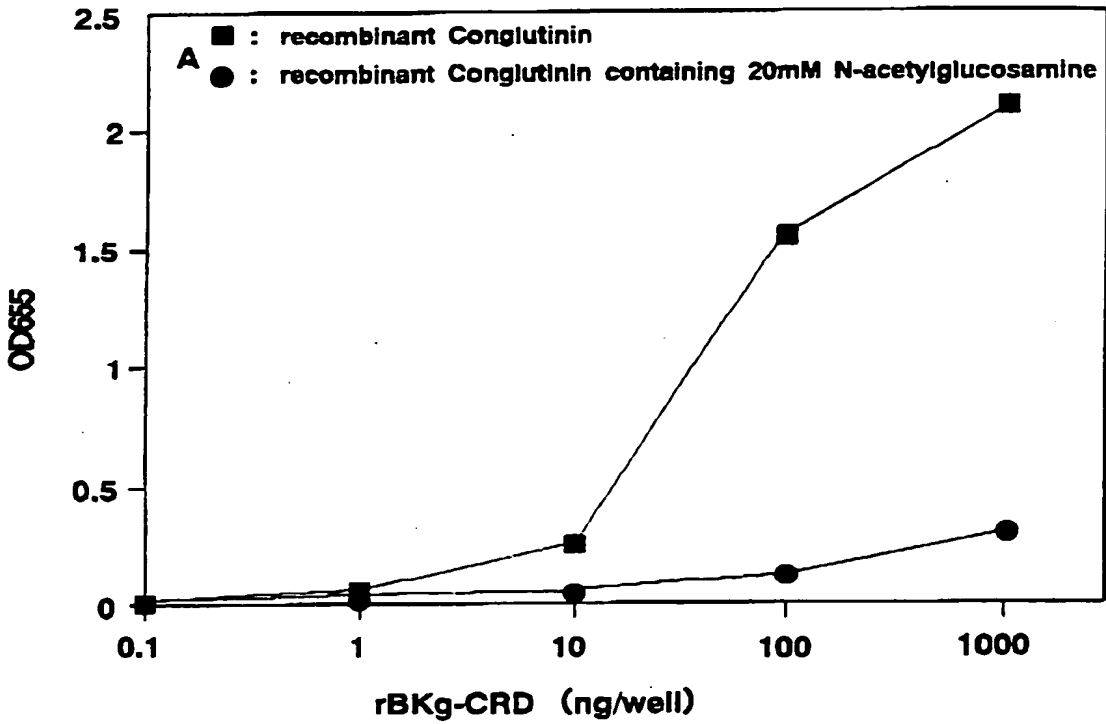

THE UNIVERSITY OF CHICAGO

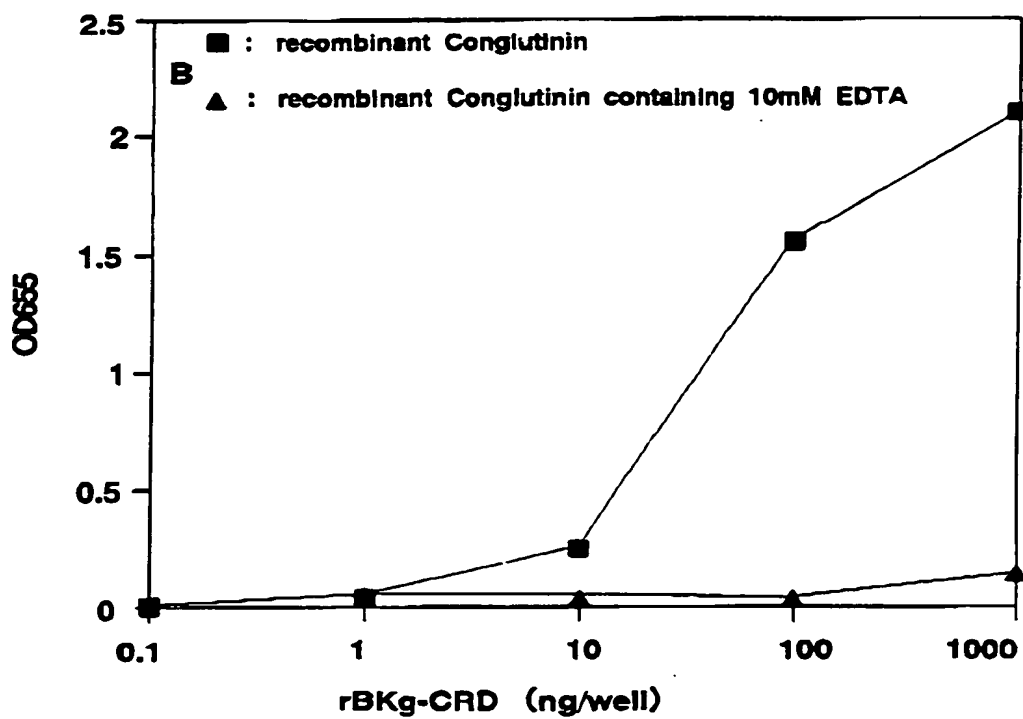

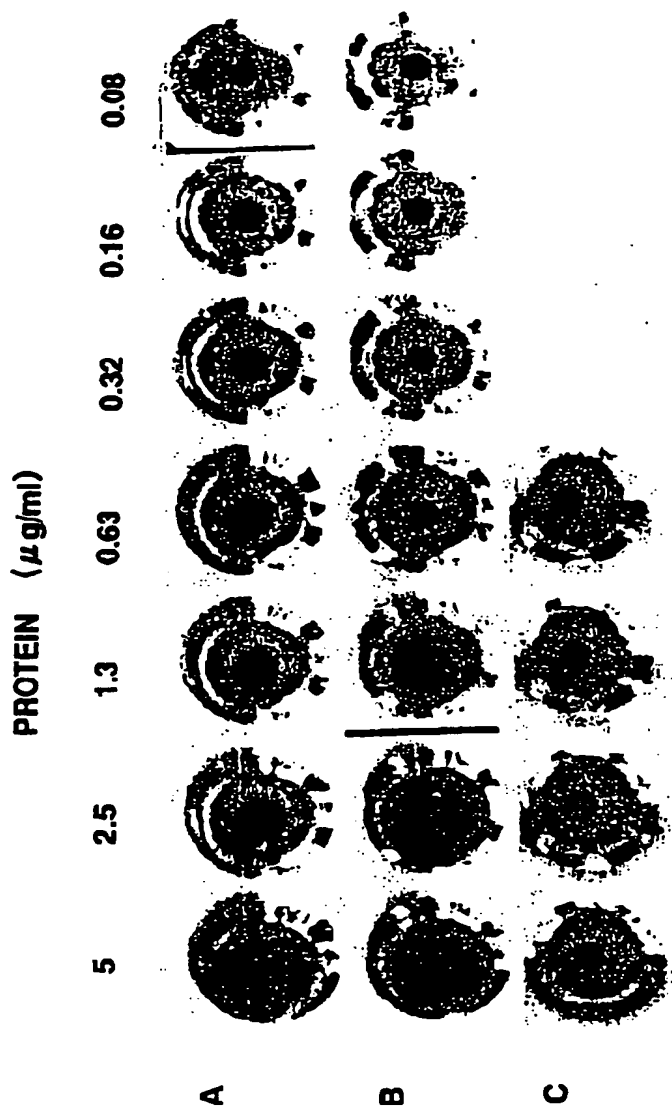


Fig.8



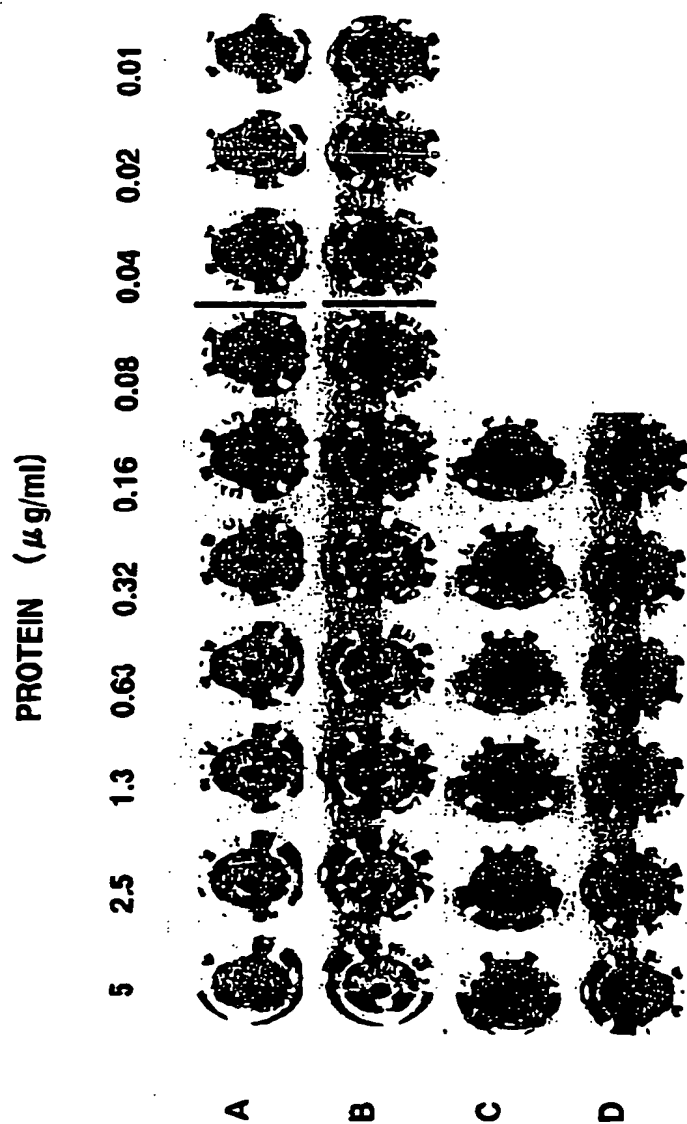




Fig.9

10007408-10807

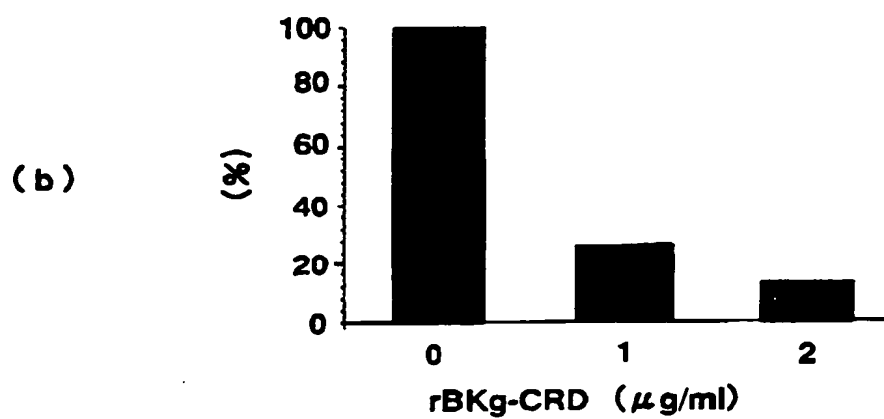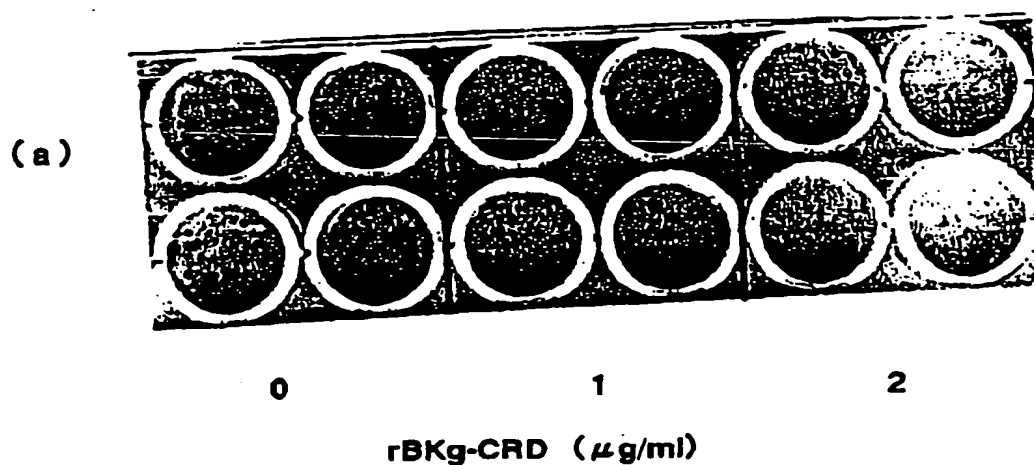


10/15


Fig.10

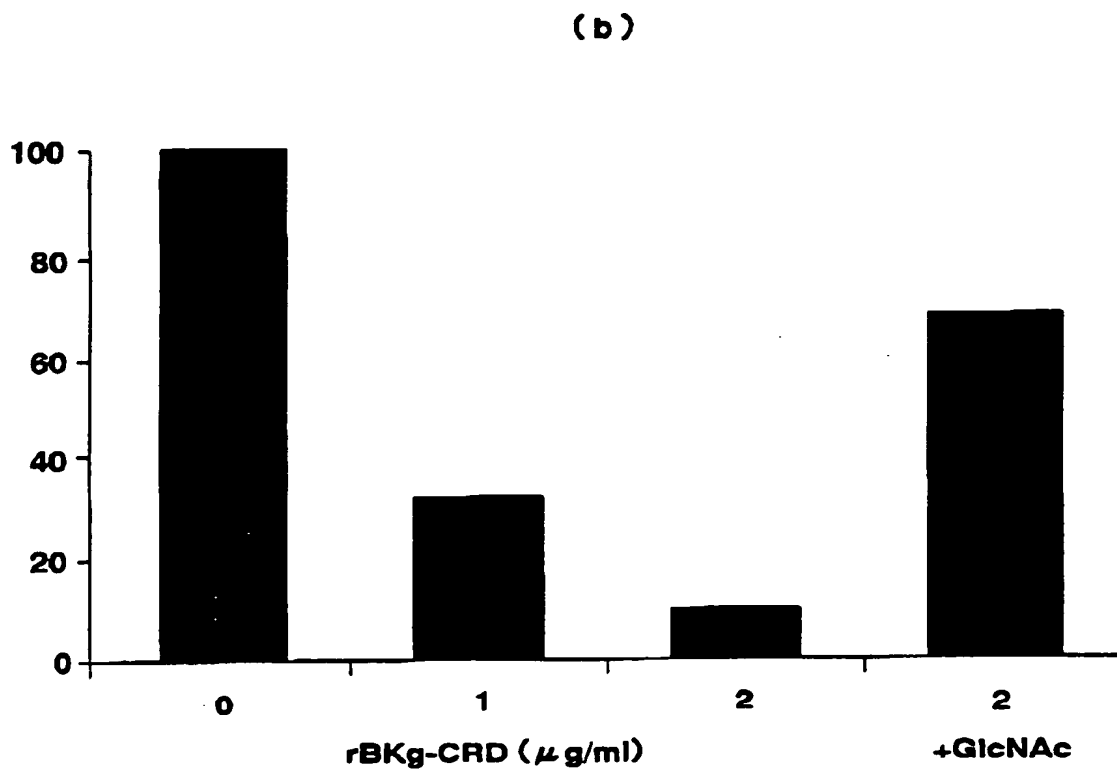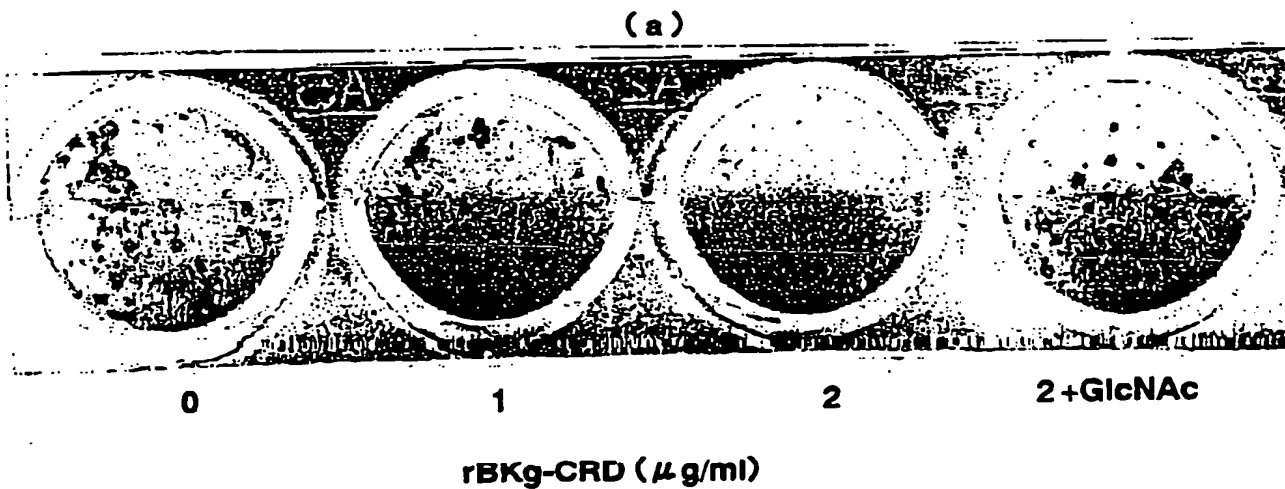


(a)

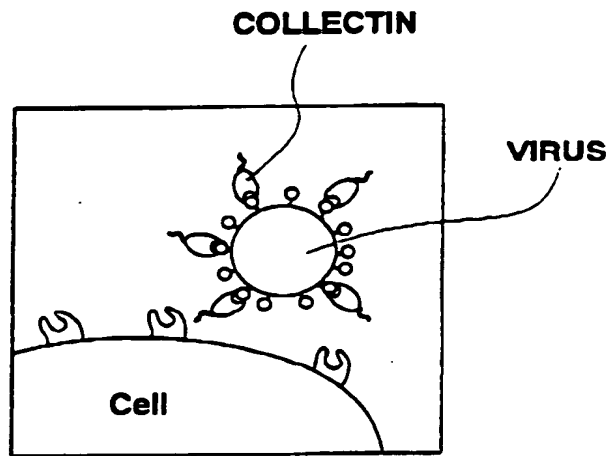

(b)

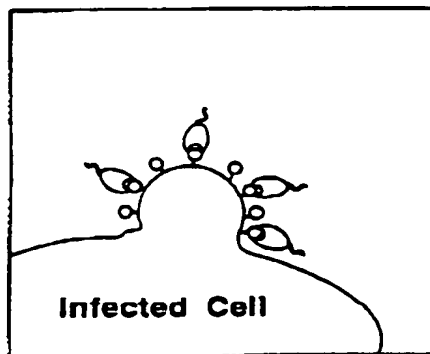

108077-8042000F

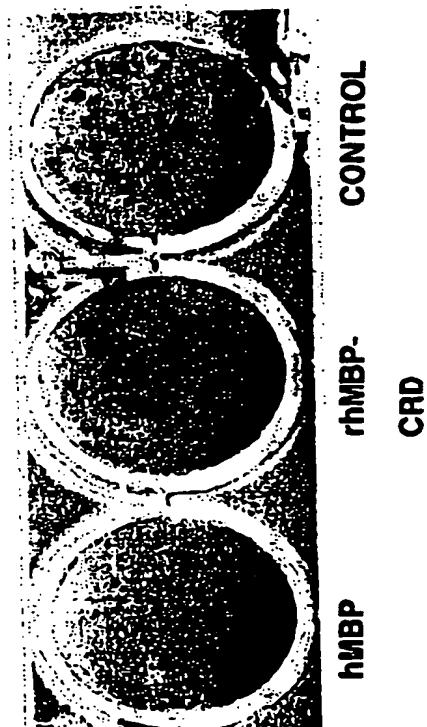

13/15

Fig.13

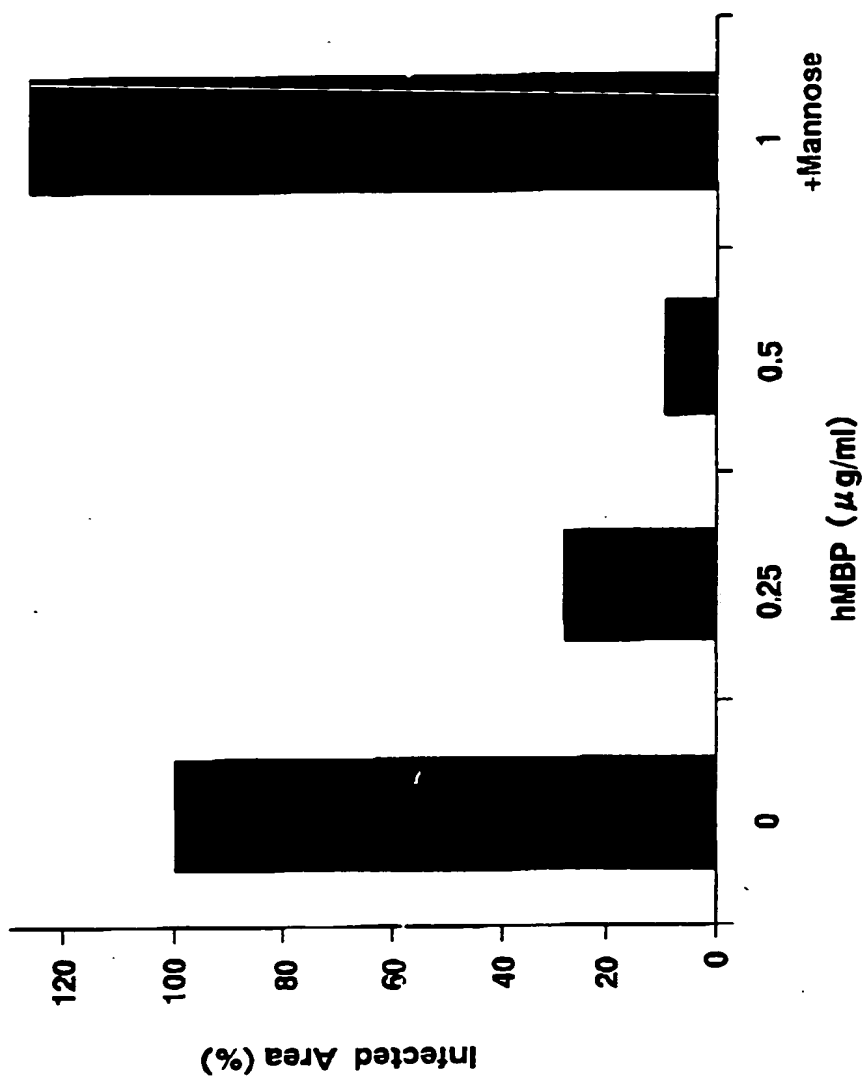


Fig.14

